


Compton Calibration

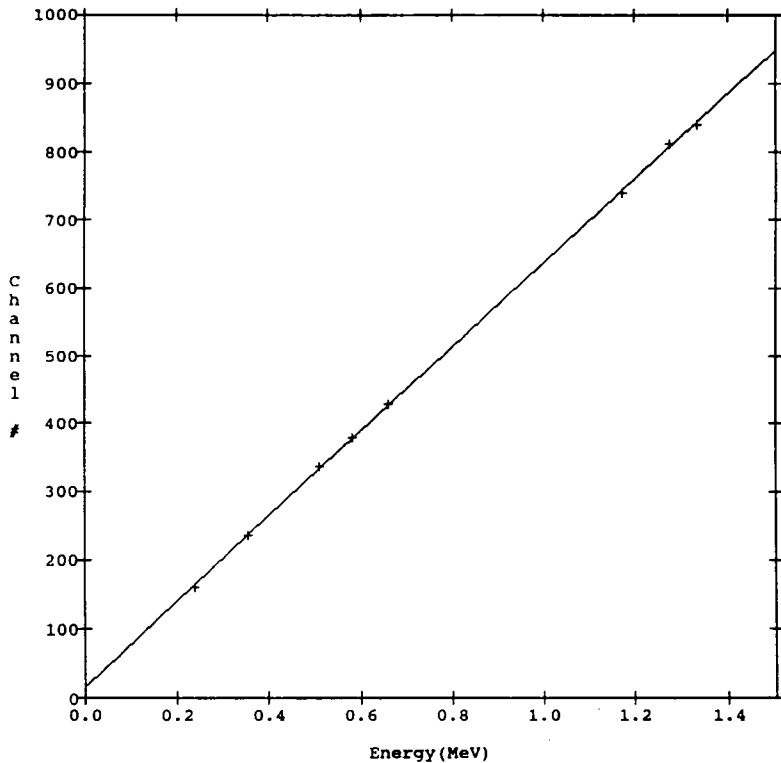

+ HV=1100 V
— 621.330038*X +16.000526

0.239 MeV	: Th 228
0.356 MeV	: Ba 133
0.511 MeV	: Na 22
0.583 MeV	: Th 228
0.662 MeV	: Cs 137
1.173 MeV	: Co 60
1.333 MeV	: Co 60
1.275 MeV	: Na 22